

SEP 10 2009

**VERIFICATION OF CALIBRATION REPORT**  
*of DataMaster cdm Breath Test Instrument*  
**State of Alaska**  
**Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program**

<b>DataMaster cdm S/N</b> <u>130176</u> ✓	
Supervisor/Operator Performing the Verification Procedure:	
Name <u>J Swartz</u>	ID# <u>4314</u> Date <u>6/4/09</u> ✓
A Agency <u>SCDL</u> Phone # <u>269-5592</u>	
Instrument Location <u>SCDL</u>	
B Alco S/N <u>SC01108</u> ✓ Target Value <u>.080</u> ✓ High Pressure <u>700 psi</u>	
Alco Test Values <u>.083</u> ✓ 1 <sup>st</sup> Alco <u>.082</u> ✓ 2 <sup>nd</sup> Alco	
Signature <u>[Signature]</u>	
(OVER)	

[Signature] 9/22/09

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Signature]  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 8th day of Oct., 2009.

[Signature] (Notary Seal Stamp)

Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

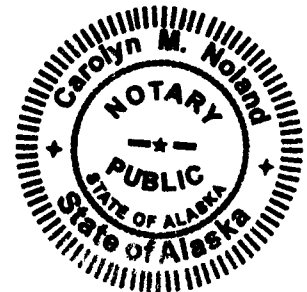

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130176 ✓

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATA MASTER cdm 130176

JUNE 04, 2009

OPERATOR'S NAME:

SWARTZ/J

OPERATOR'S NUMBER: 4314

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

L

O.L. #: L

DEPT/AGENCY: AAP1

CASE/REPORT:

TEST TYPE: U

ALCO TARGET VALUE: .000

ALCO S/N: SCOTT00

### BREATH ANALYSIS

.000 ADJUSTED FOR 30.03 in

ALCO TARGET .000 16:14

BLANK TEST .000 16:15

INTERNAL STANDARD VERIFIED 16:15

ALCO TO 30.01 in .003 16:15

BLANK TEST .000 16:16

SUBJECT SAMPLE .000 16:16

BLANK TEST .000 16:17

ALCO TO 30.01 in .002 16:17

BLANK TEST .000 16:18

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATA MASTER cdm 130176

JUNE 04, 2009

TIME 16:12

### DIAGNOSTIC CHECK

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 01/00/09

HEATERS

SAMPLE CHAMBER: 40c

BREATH TUBE: 41c

BAROMETER: 30.01 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

### PRINTER TEST

! " # \$ % ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { | } ~